




Fig. I

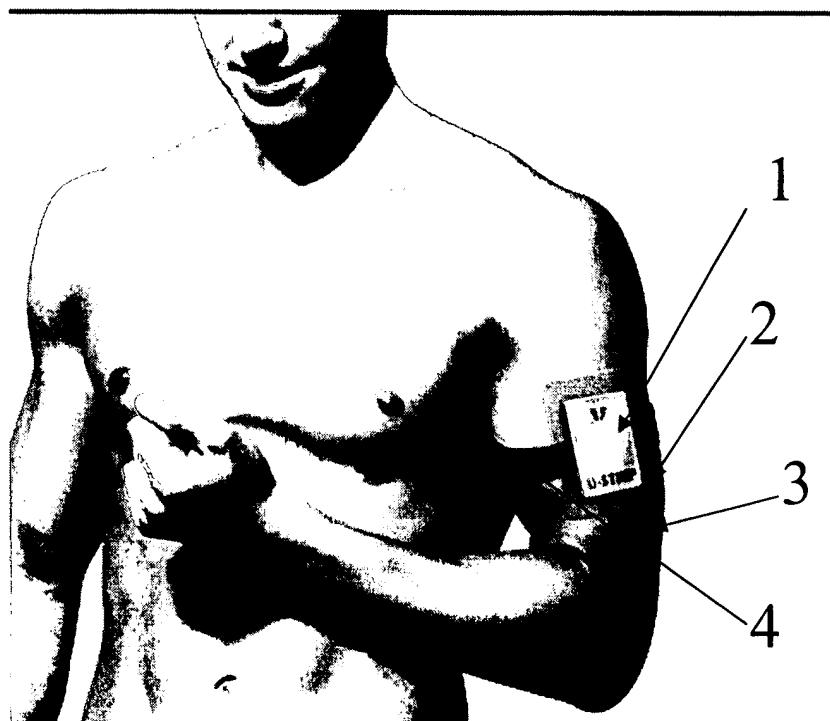


*Fig. 2*

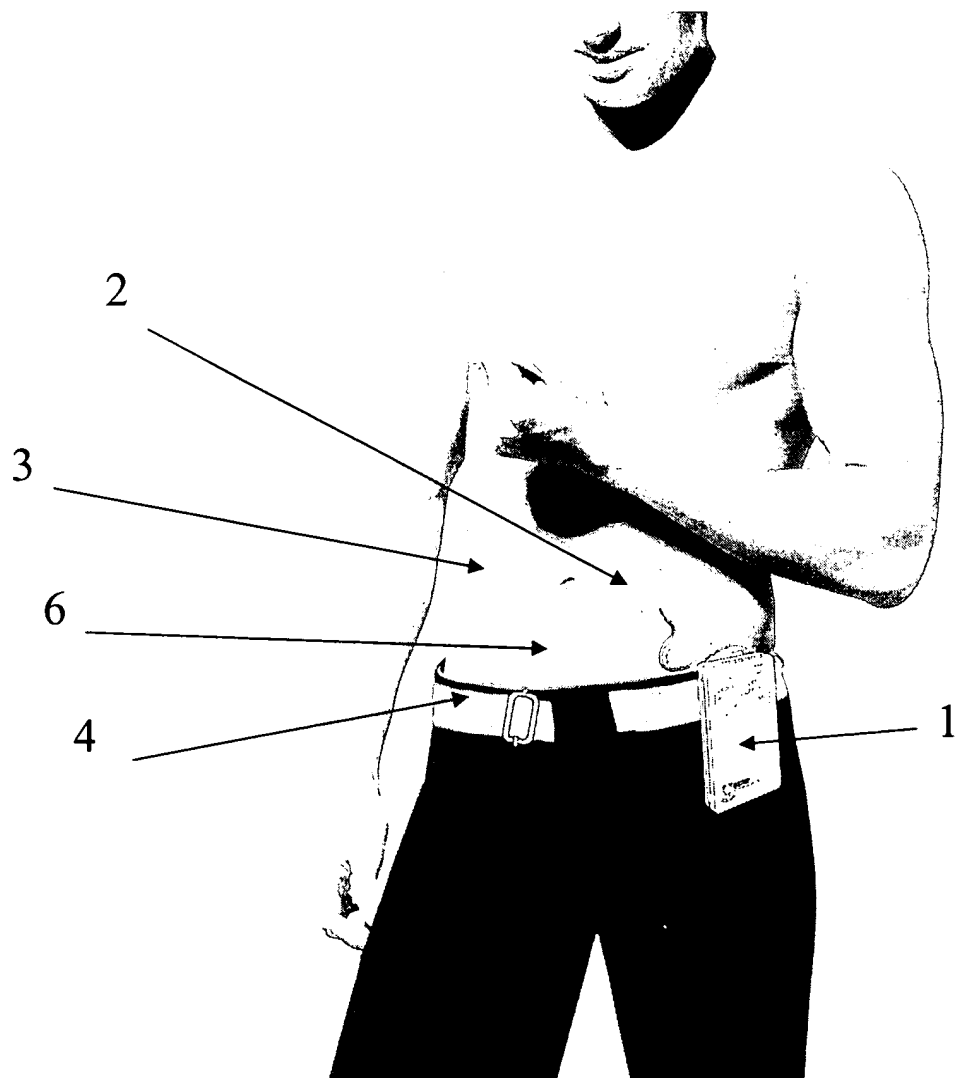


*Fig. 3*

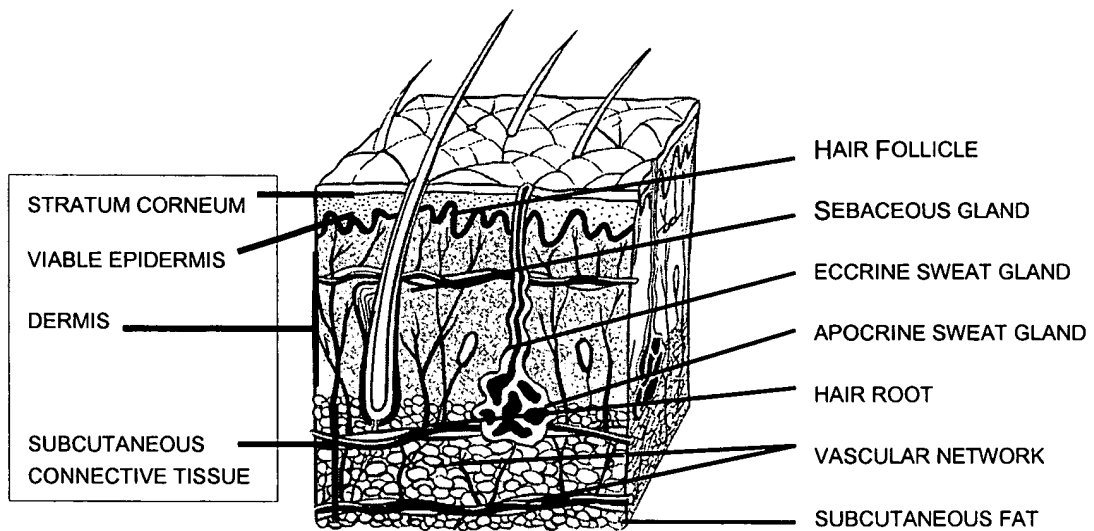


***Fig. 4A***

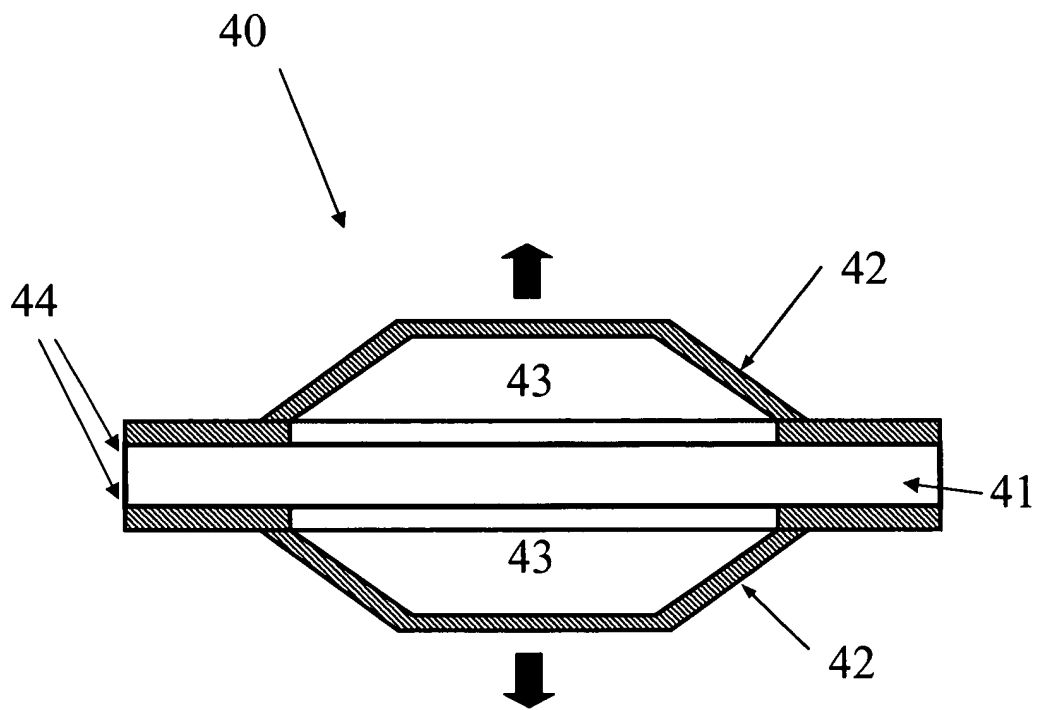


***Fig. 4B***

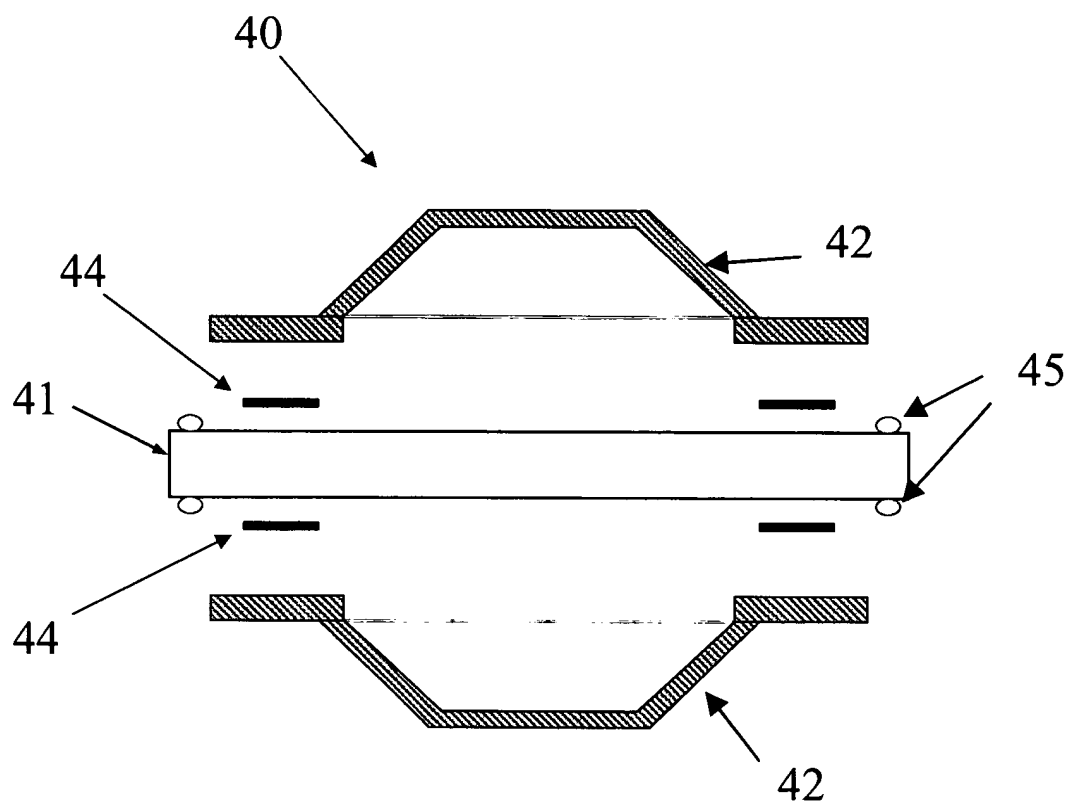


*Fig. 4C*

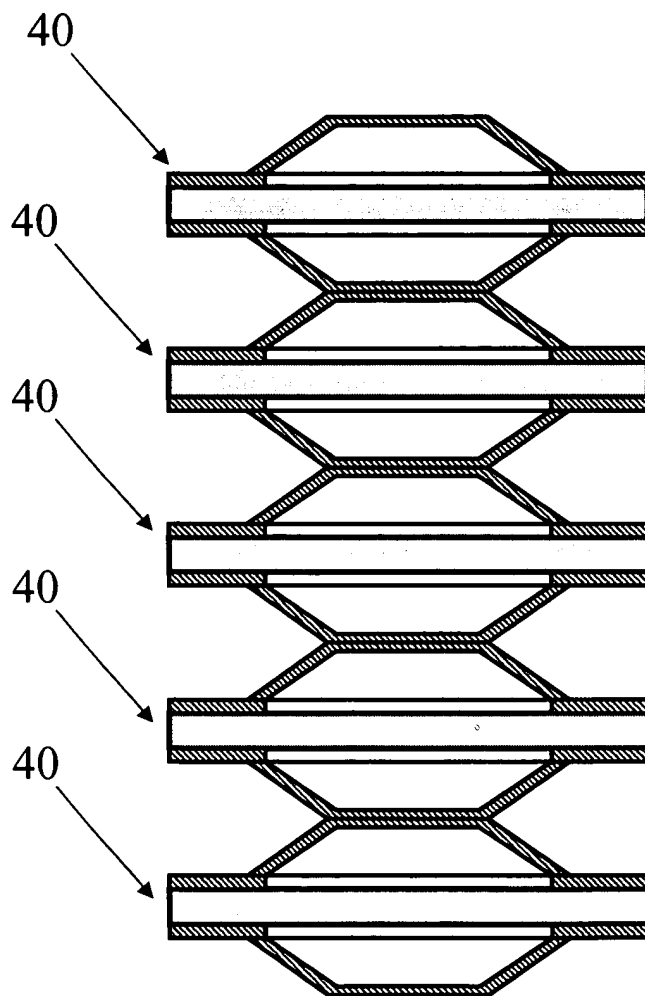

*Fig. 5A*

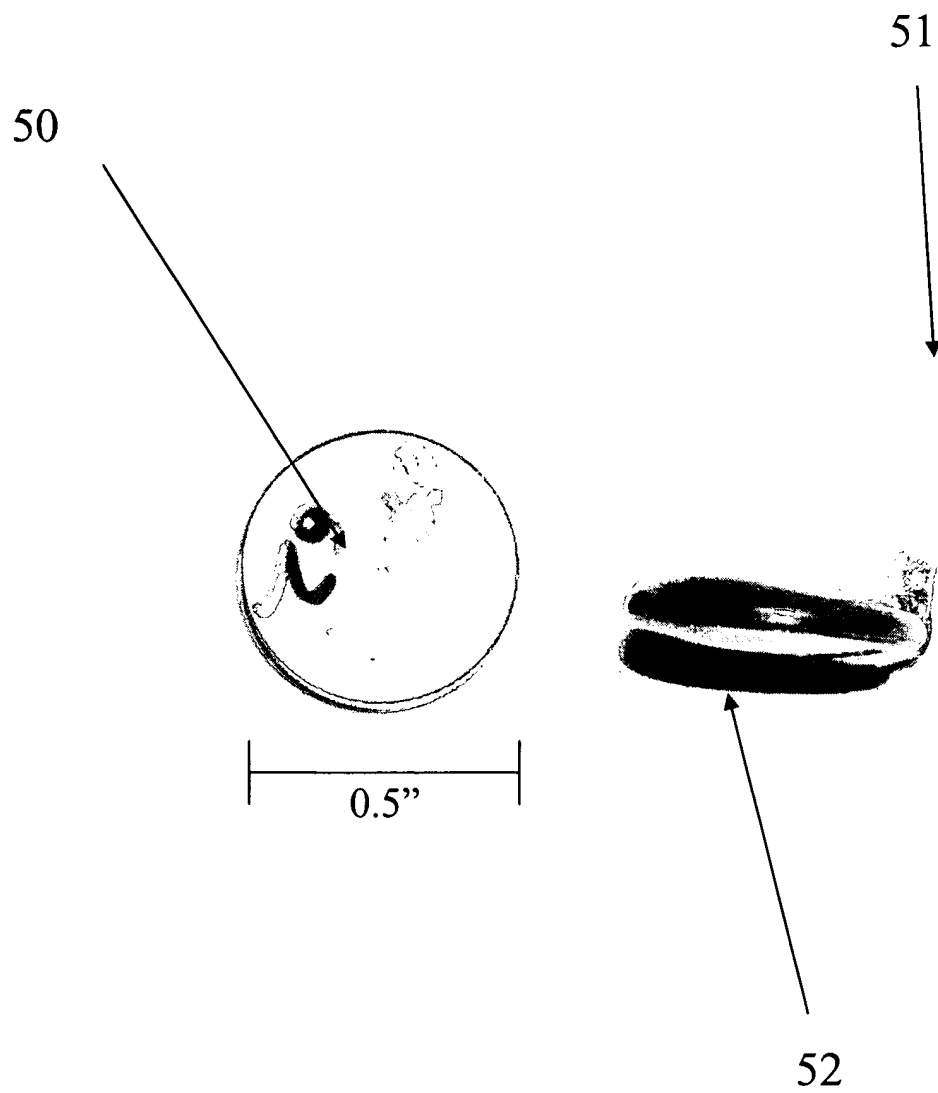


***Fig. 5B***

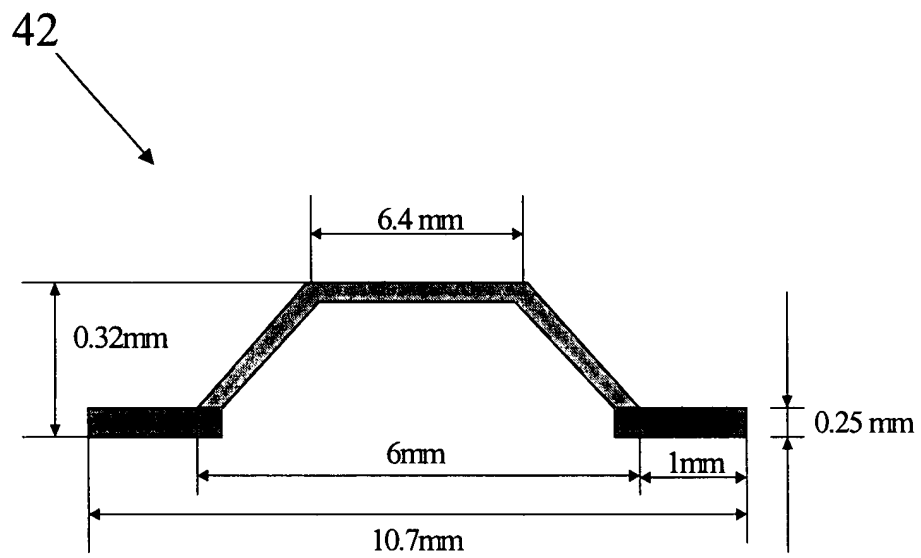




*Fig. 6*

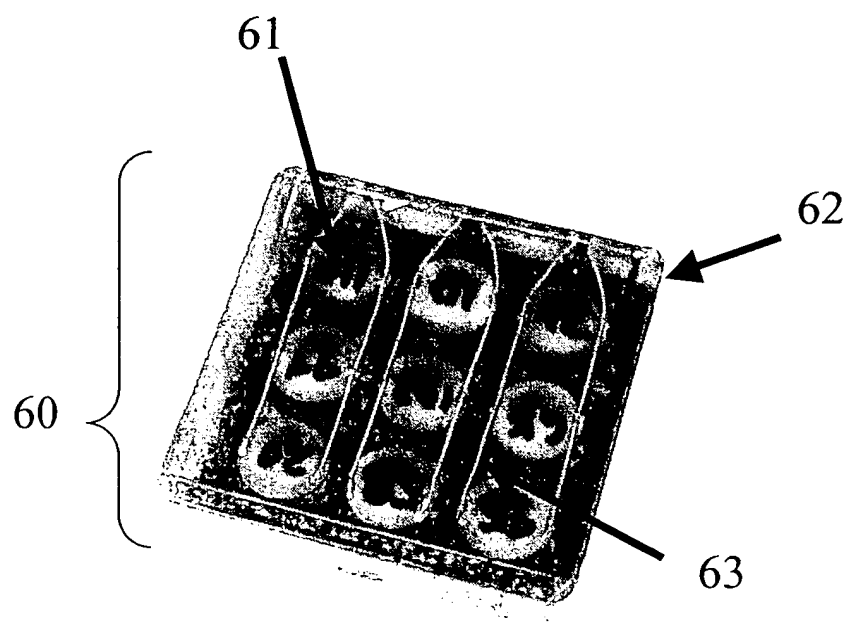

***Fig. 7***

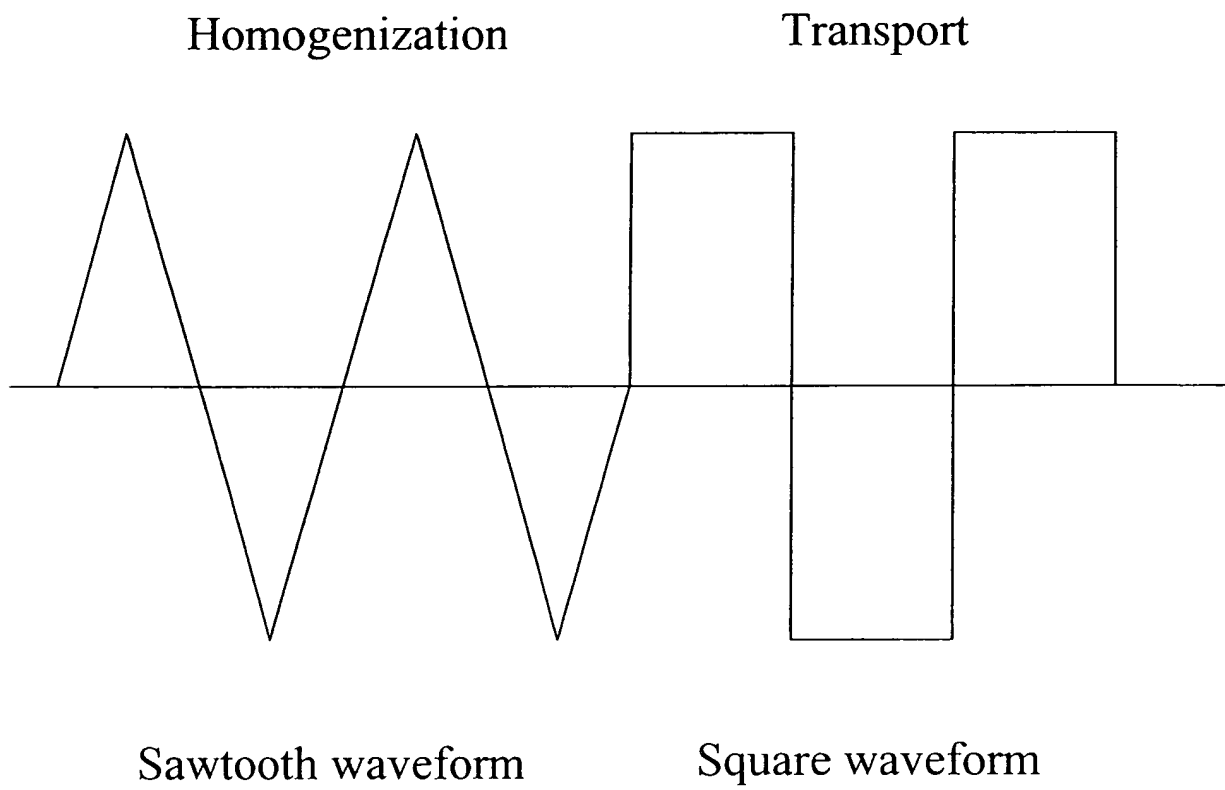

**Fig. 8**

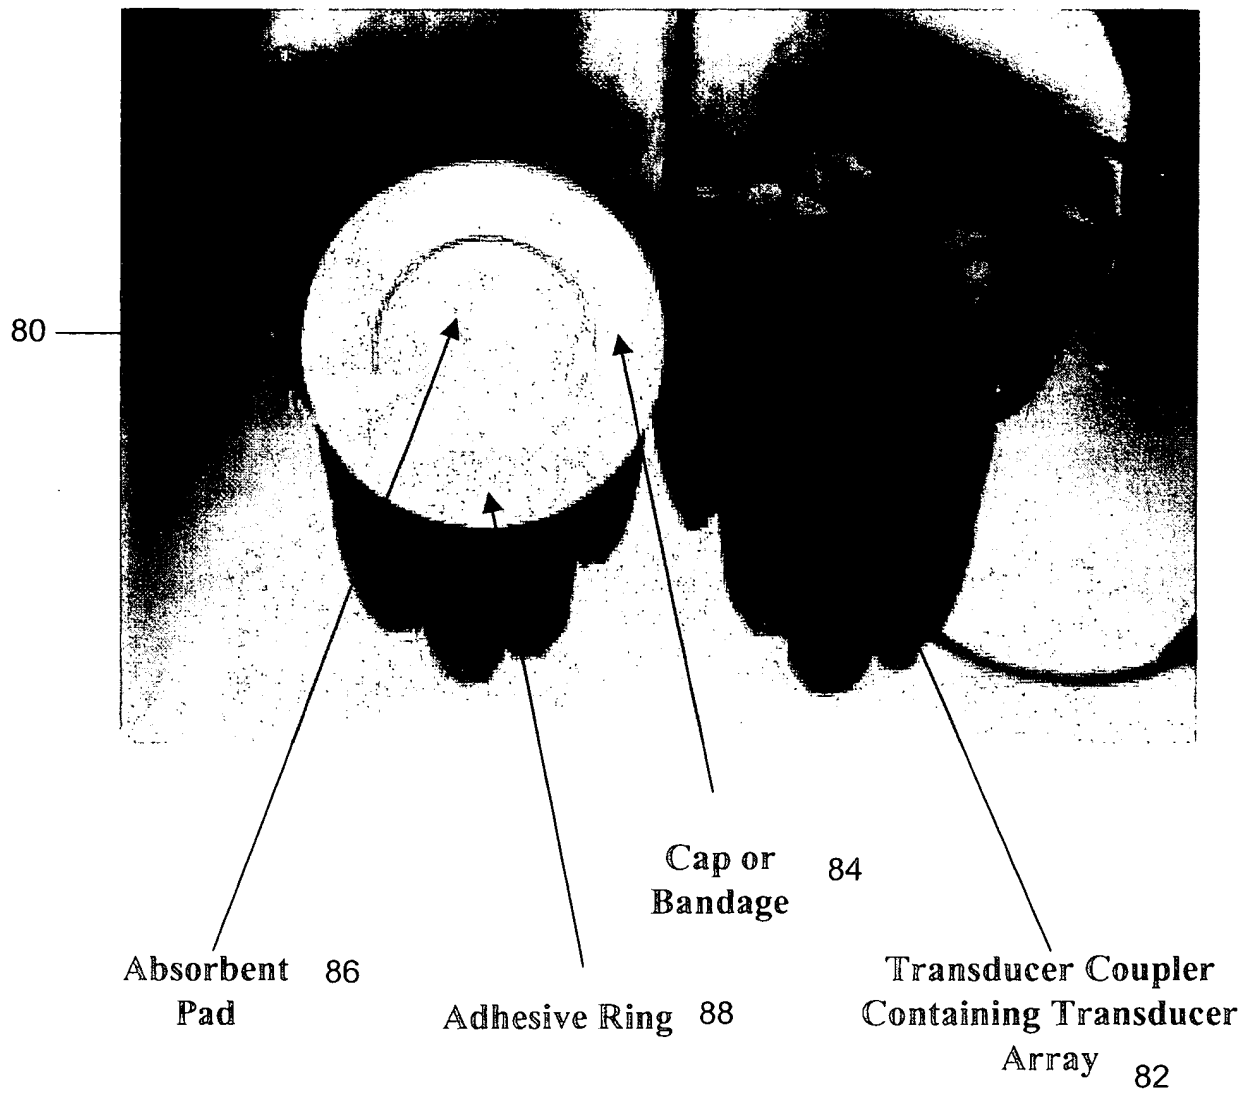
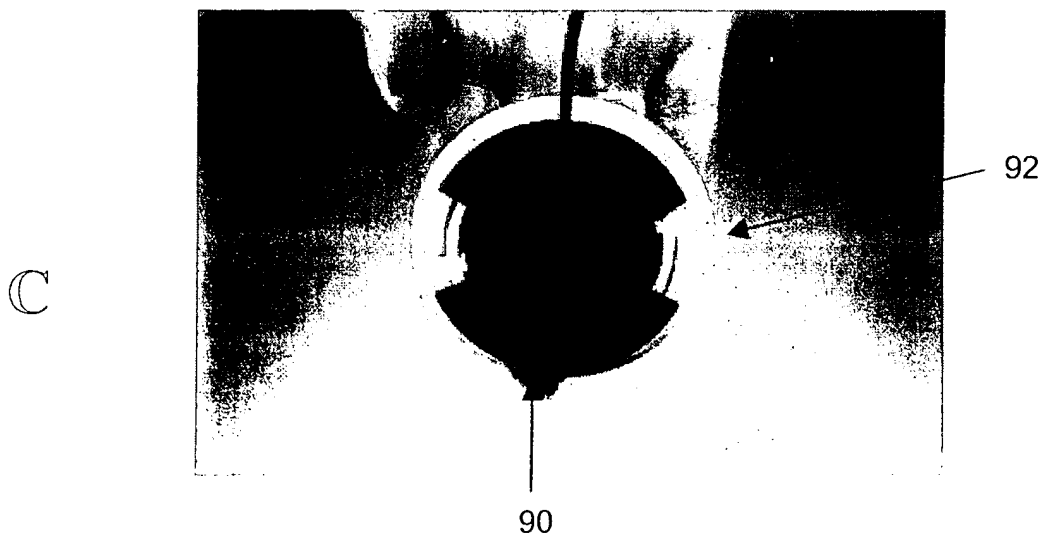


Fig. 9



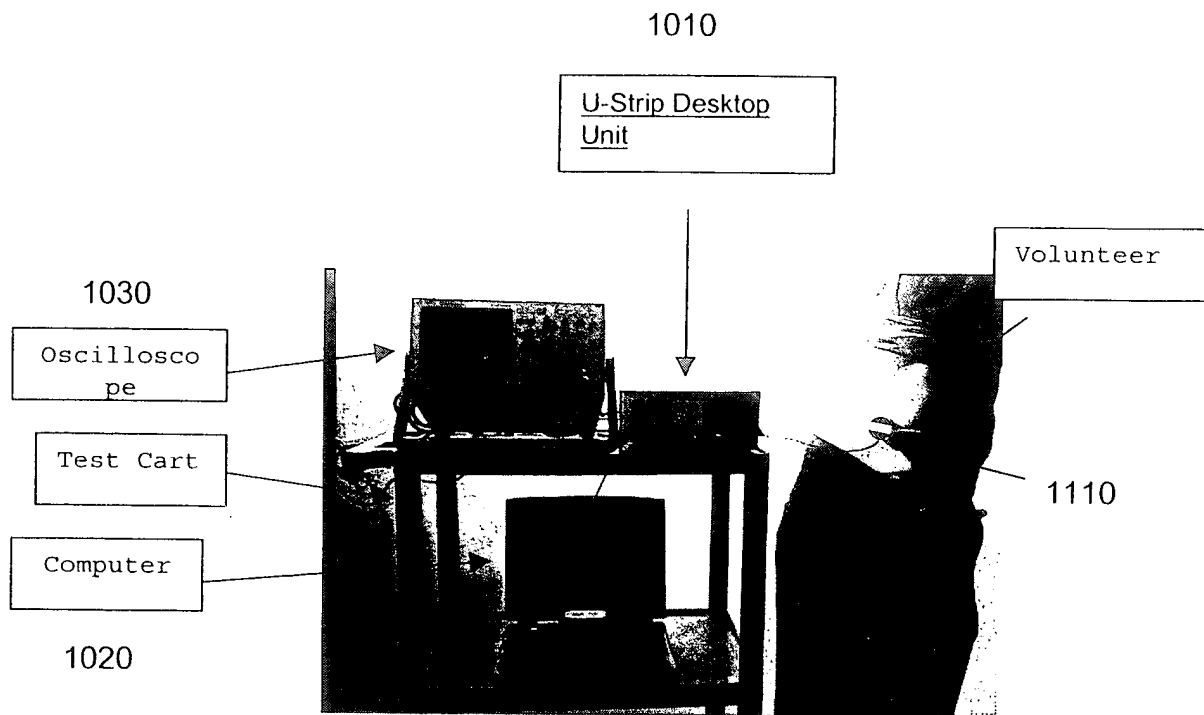
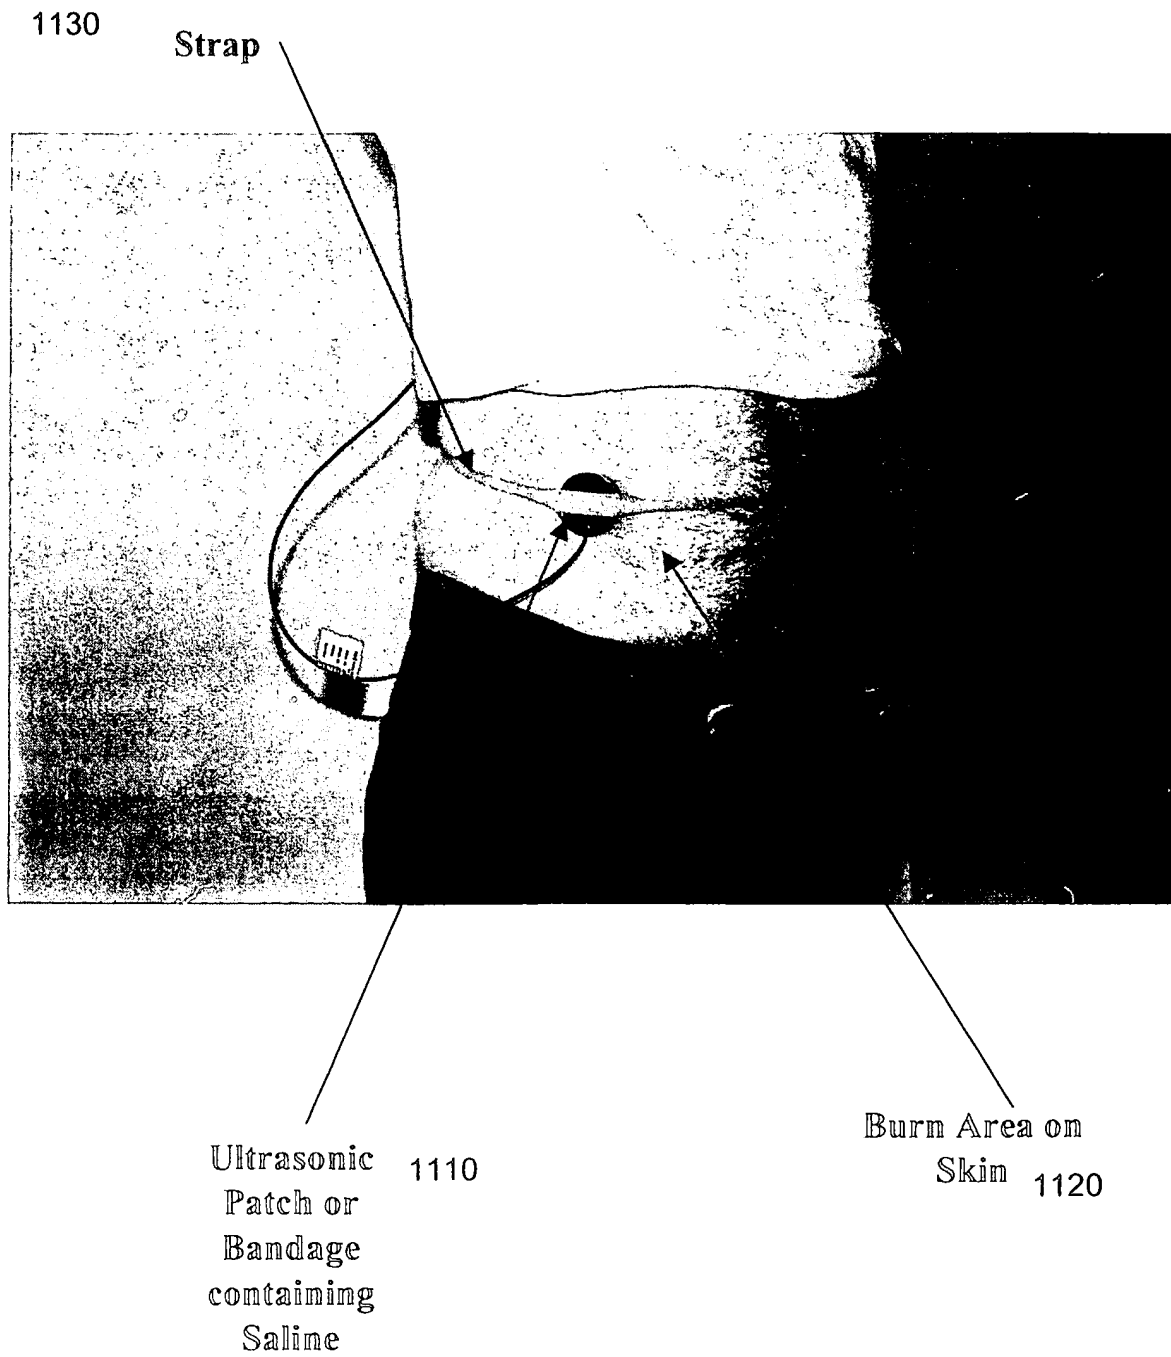


FIG. 10: U-Strip Test Set Rig.

**Fig. 11**



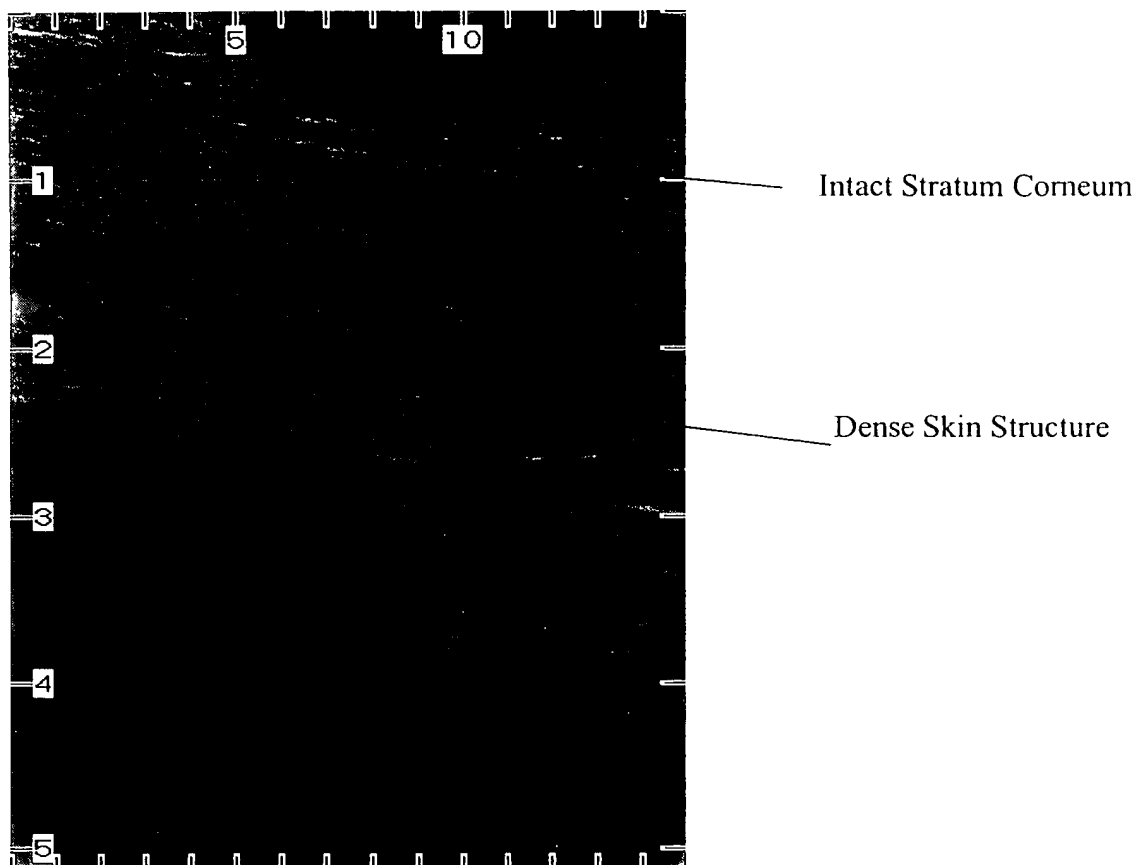


Figure 12 A

Image 1

Scan #21 Baseline Scan of Abdomen Control Site

Depth capture 5.1 mm

Control Scan (No Ultrasound), Saline left  
upon Skin surface

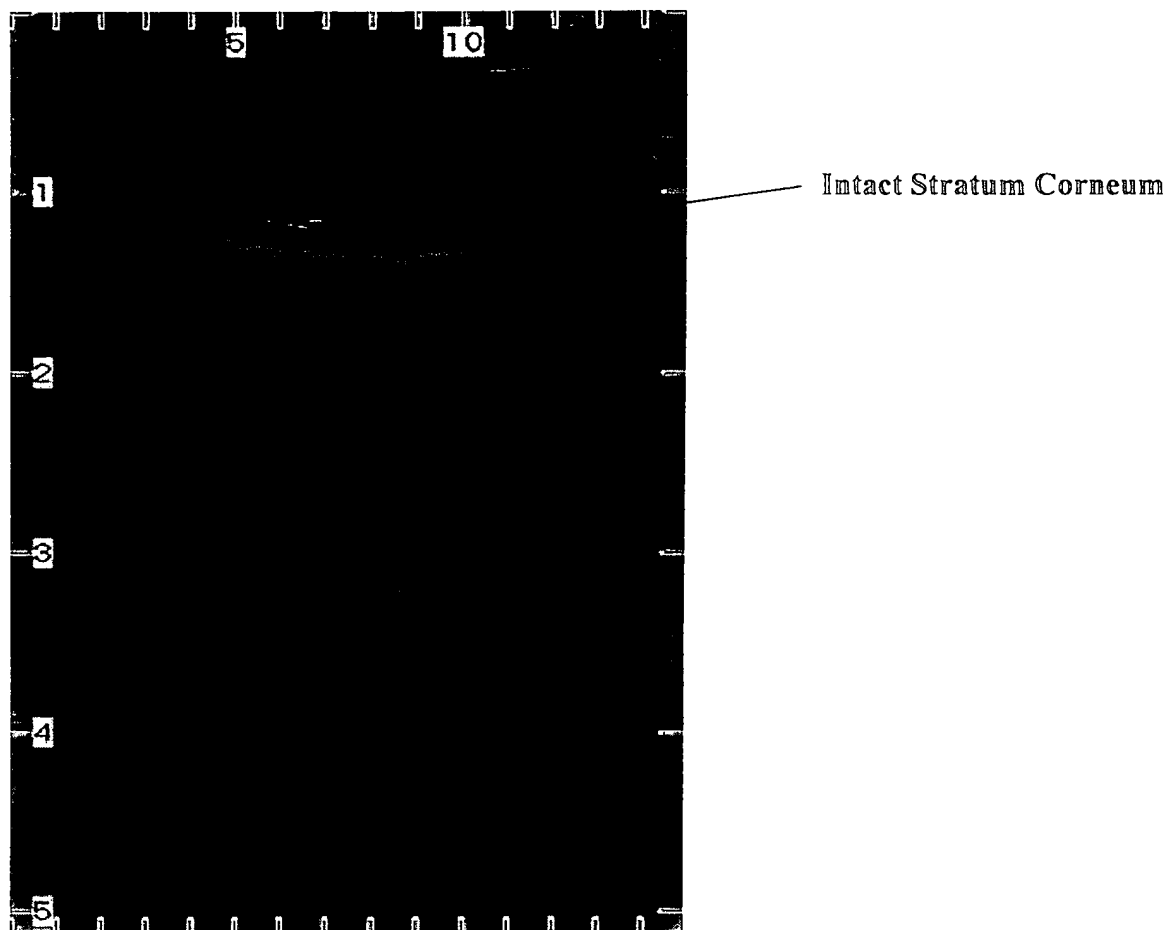


Figure 12 B

Image 2

#28 45 min with unplowed transducer.

Depth capture 5.1mm



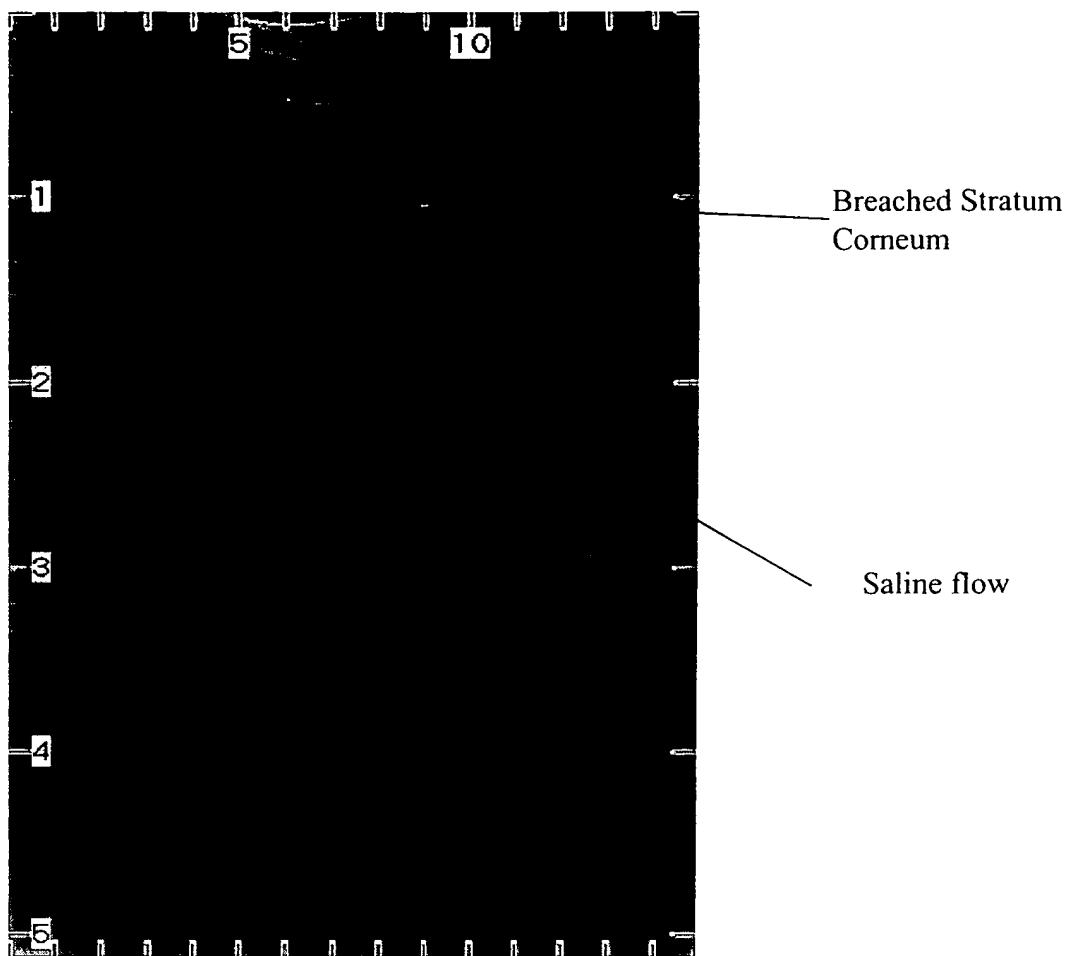


Figure 12 C

Image 3

Scan #25: 45 min treated

(#5 set, # 8 transducer)

Saline Pushed By Ultrasound To 5.2 mm Depth through Abdominal Skin

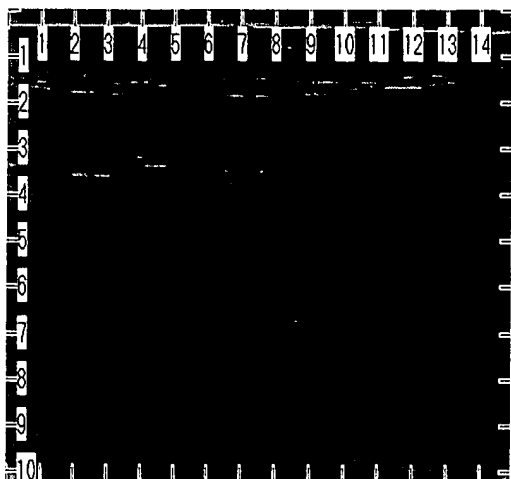


Figure 12 D

Image 4

Scan# 32 – 90 min untreated.  
Unpowered transducer.

Depth capture 10.2mm

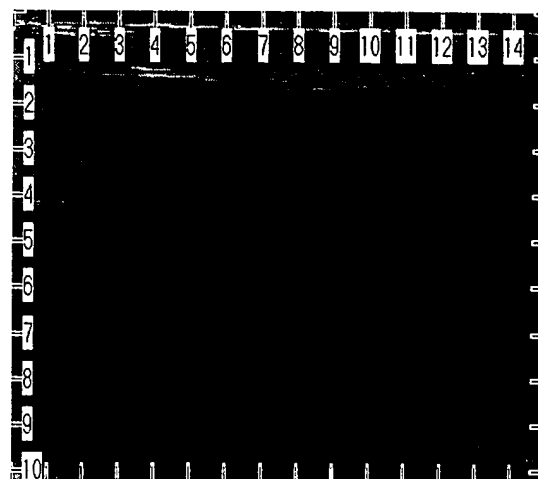


Figure 12 E

Image 5

Scan # 33 – 90 min treated.  
Powered transducer.

Depth capture 10.2mm

**This Page is Inserted by IFW Indexing and Scanning  
Operations and is not part of the Official Record**

## **BEST AVAILABLE IMAGES**

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images include but are not limited to the items checked:

- ☐ BLACK BORDERS
- ☐ IMAGE CUT OFF AT TOP, BOTTOM OR SIDES
- ☐ FADED TEXT OR DRAWING
- ☐ BLURRED OR ILLEGIBLE TEXT OR DRAWING
- ☐ SKEWED/SLANTED IMAGES
- ☒ COLOR OR BLACK AND WHITE PHOTOGRAPHS
- ☐ GRAY SCALE DOCUMENTS
- ☐ LINES OR MARKS ON ORIGINAL DOCUMENT
- ☐ REFERENCE(S) OR EXHIBIT(S) SUBMITTED ARE POOR QUALITY
- ☐ OTHER: \_\_\_\_\_

**IMAGES ARE BEST AVAILABLE COPY.**

**As rescanning these documents will not correct the image problems checked, please do not report these problems to the IFW Image Problem Mailbox.**